


Sample Name: M-6-15-17

=====

Acq. Operator : SYSTEM Seq. Line : 7
Acq. Instrument : Agilent HPLC Location : 8
Injection Date : 6/15/2018 3:13:47 PM Inj : 1
Inj Volume : 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.000 µl
Acq. Method : D:\2018\TEST\DATA\20180615\20180615-01 2018-06-15 12-54-27\5-(10)-100(5)-1-40-210.M
Last changed : 6/15/2018 12:54:27 PM by SYSTEM
Analysis Method : D:\2018\TEST\DATA\20180615\20180615-01 2018-06-15 12-54-27\5-(10)-100(5)-1-40-210.M (Sequence Method)
Last changed : 6/15/2018 3:44:58 PM by SYSTEM
(modified after loading)
Additional Info : Peak(s) manually integrated

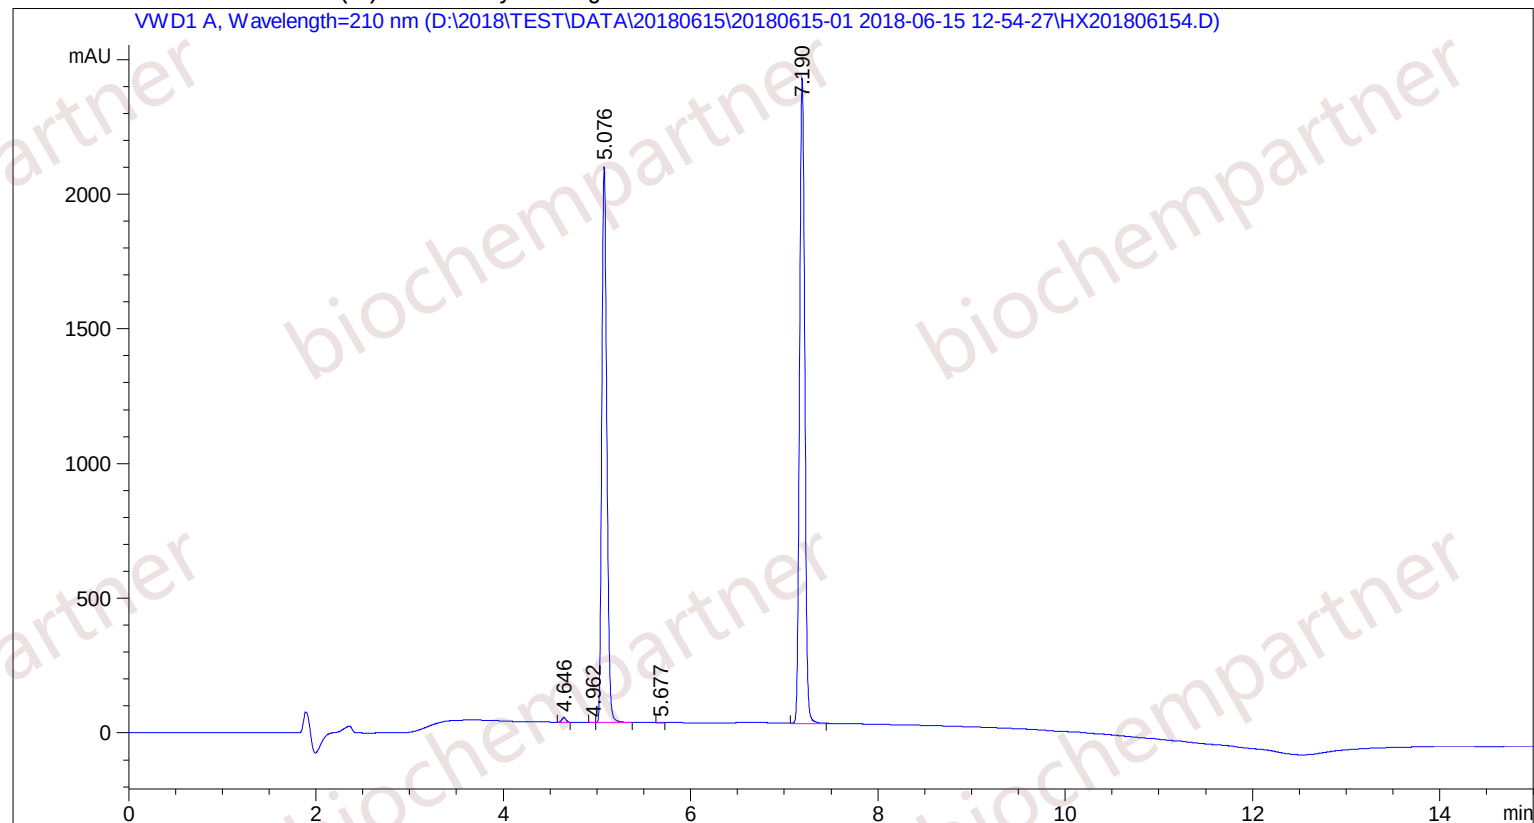

=====

Area Percent Report

=====

Sorted By : Signal
Multiplier : 1.0000
Dilution : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: VWD1 A, Wavelength=210 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	4.646	MM	0.0509	53.09190	17.38297	0.3097
2	4.962	MF	0.0481	1.65043	5.72072e-1	9.626e-3
3	5.076	FM	0.0635	7865.35791	2065.13843	45.8745
4	5.677	MM	0.0603	8.77344	2.42459	0.0512

Sample Name: M-6-15-17

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
5	7.190	MM	0.0641	9216.51465	2397.64795	53.7551

Totals : 1.71454e4 4483.16601

=====
*** End of Report ***