


Sample Name: M-6-21-12

```

=====
Acq. Operator   : SYSTEM                       Seq. Line   :    4
Acq. Instrument : Agilent HPLC                 Location    :    6
Injection Date  : 6/21/2018 2:57:04 PM       Inj         :    1
                                           Inj Volume  : 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 3.500 µl
Method          : D:\2018\TEST\DATA\20180621\20180621-02 2018-06-21 13-46-42\5-(10)-100(5)-1-40-210.M (Sequence Method)
Last changed    : 6/21/2018 1:46:42 PM by SYSTEM
Additional Info  : Peak(s) manually integrated
=====
    
```

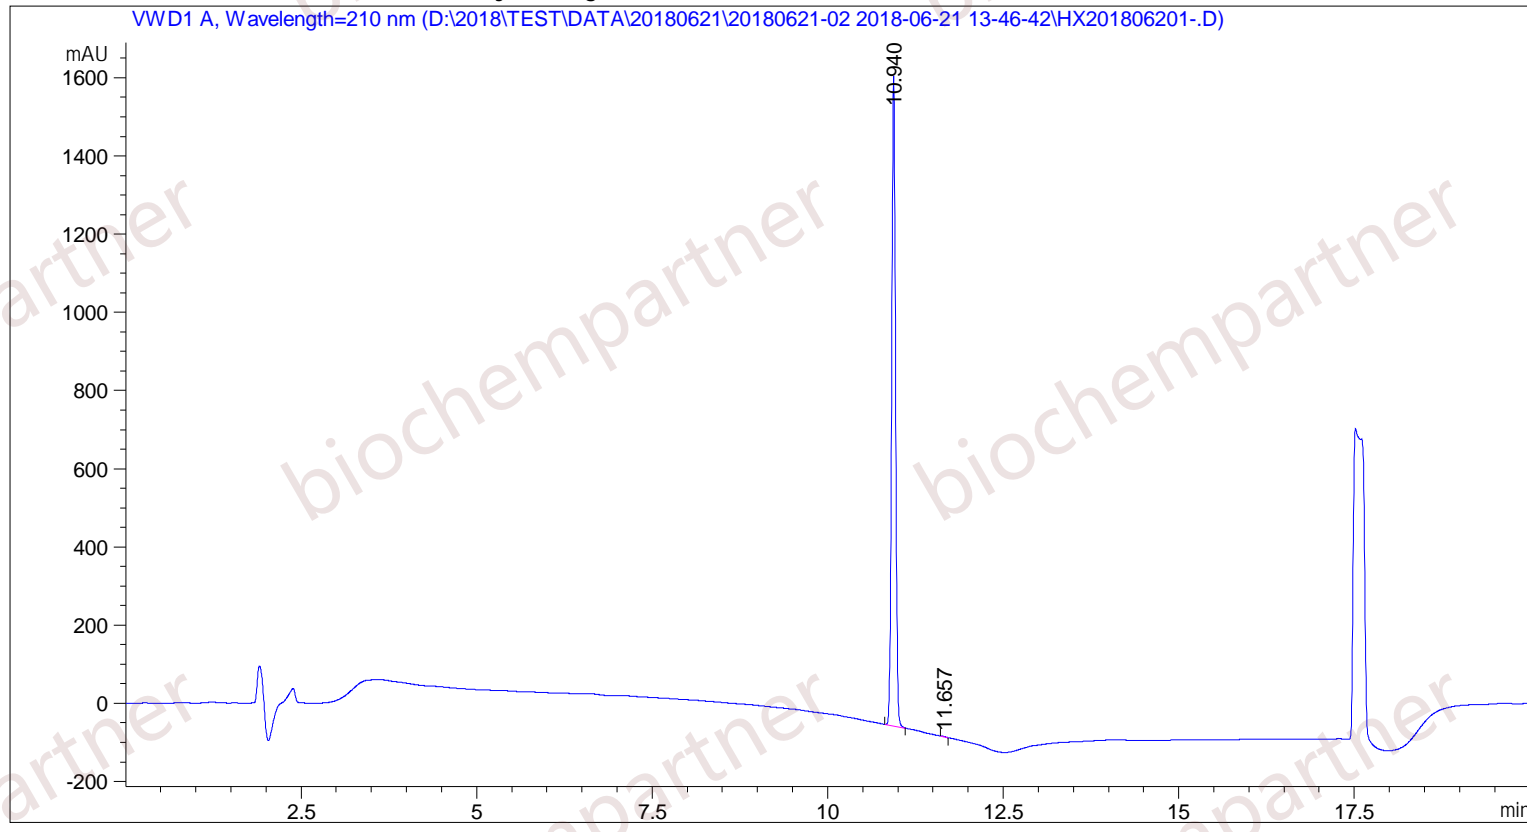

=====
Area Percent Report
=====

```

Sorted By       :      Signal
Multiplier      :      1.0000
Dilution        :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=210 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	10.940	MM	0.0631	6303.76709	1664.11133	99.9310
2	11.657	MM	0.0657	4.35368	1.10511	0.0690

Totals : 6308.12077 1665.21644

=====
*** End of Report ***