


Sample Name:

```

=====
Acq. Operator   : SYSTEM                               Seq. Line :    1
Acq. Instrument : Agilent HPLC                         Location  :   52
Injection Date  : 7/18/2018 4:09:00 PM                 Inj       :    1
                                                    Inj Volume: 5.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl
Acq. Method     : D:\2018\TEST\DATA\20180718\20180718-04 2018-07-18 16-06-39\5-(10)-100(5)-1-40-210.M
Last changed    : 7/18/2018 4:06:39 PM by SYSTEM
Analysis Method : D:\2018\TEST\DATA\20180718\20180718-04 2018-07-18 16-06-39\5-(10)-100(5)-1-40-210.M (Sequence Method)
Last changed    : 7/18/2018 4:45:17 PM by SYSTEM
                  (modified after loading)
Additional Info : Peak(s) manually integrated
    
```

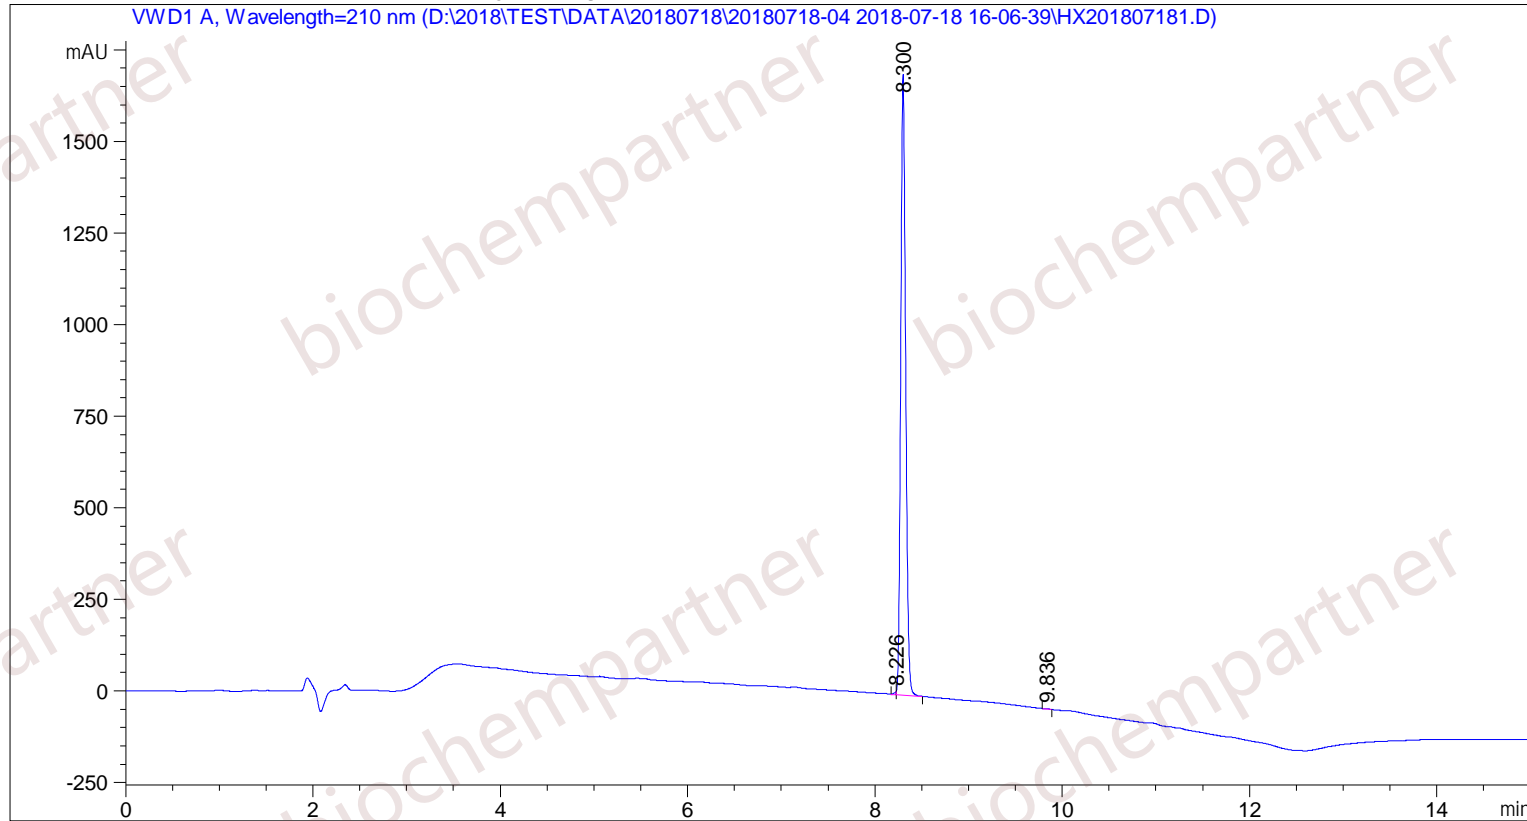

Area Percent Report

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
    
```

Signal 1: VWD1 A, Wavelength=210 nm

Peak #	RetTime [min]	Type	Width [min]	Area [mAU*s]	Height [mAU]	Area %
1	8.226	MF	0.0274	12.73258	7.74575	0.1994
2	8.300	FM	0.0625	6366.19678	1696.48218	99.7182
3	9.836	MM	0.0686	5.25555	1.27660	0.0823

Sample Name:

Totals : 6384.18491 1705.50452

=====
*** End of Report ***